

Figure 1

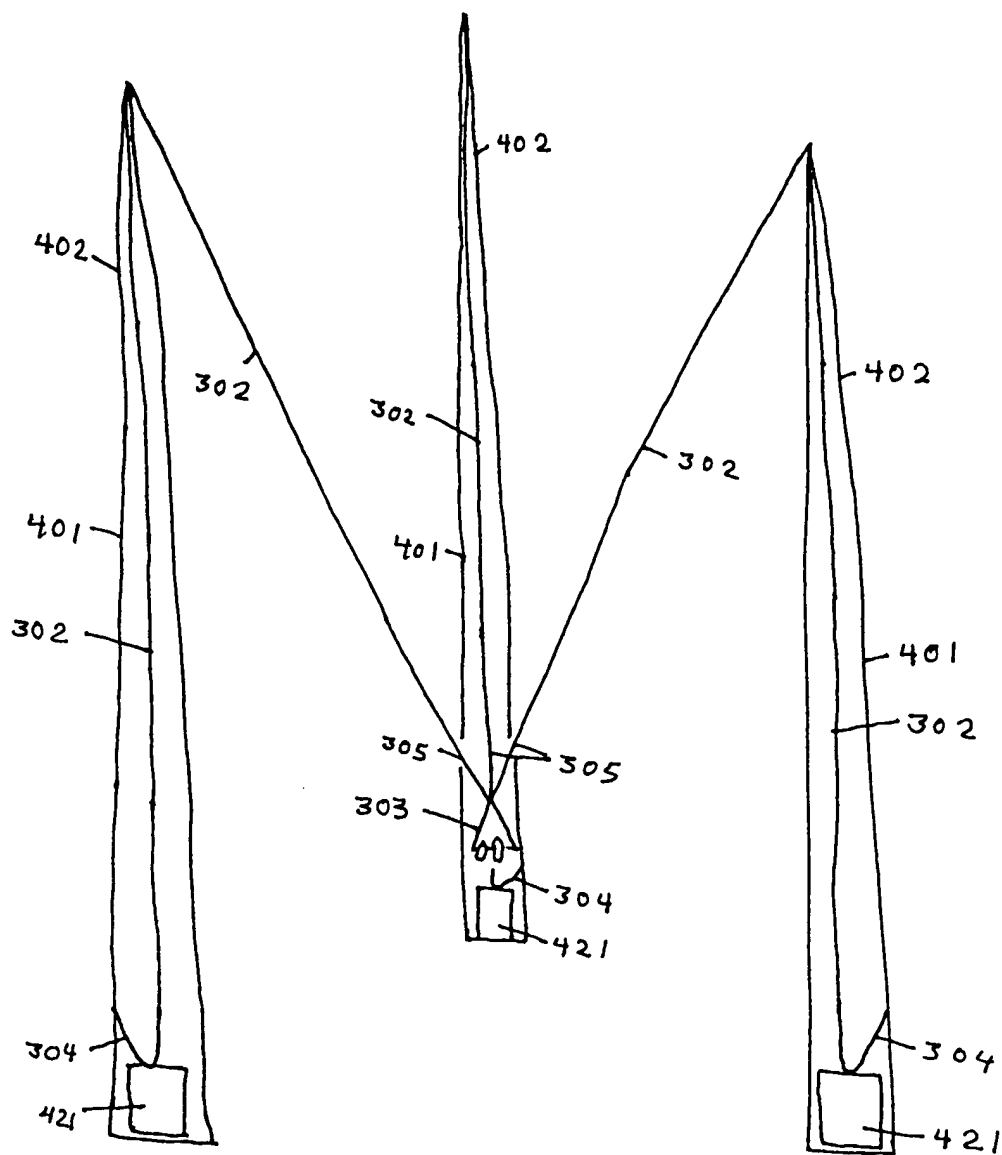


Figure 2

413 410 411 414 404 415 403 409 304 417 416 422 412

Figure 3



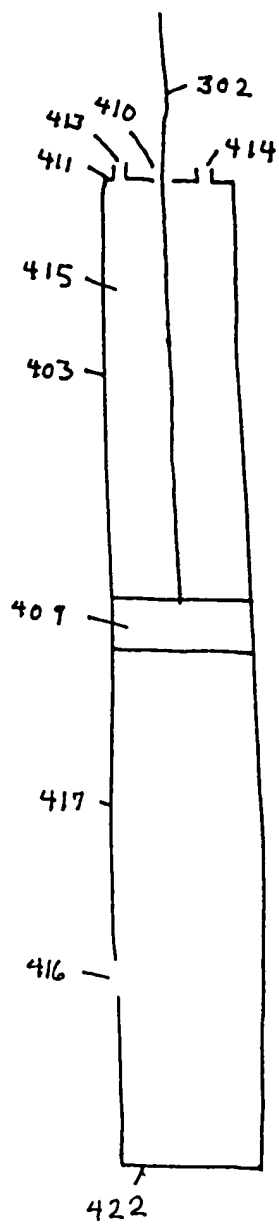


Figure 5

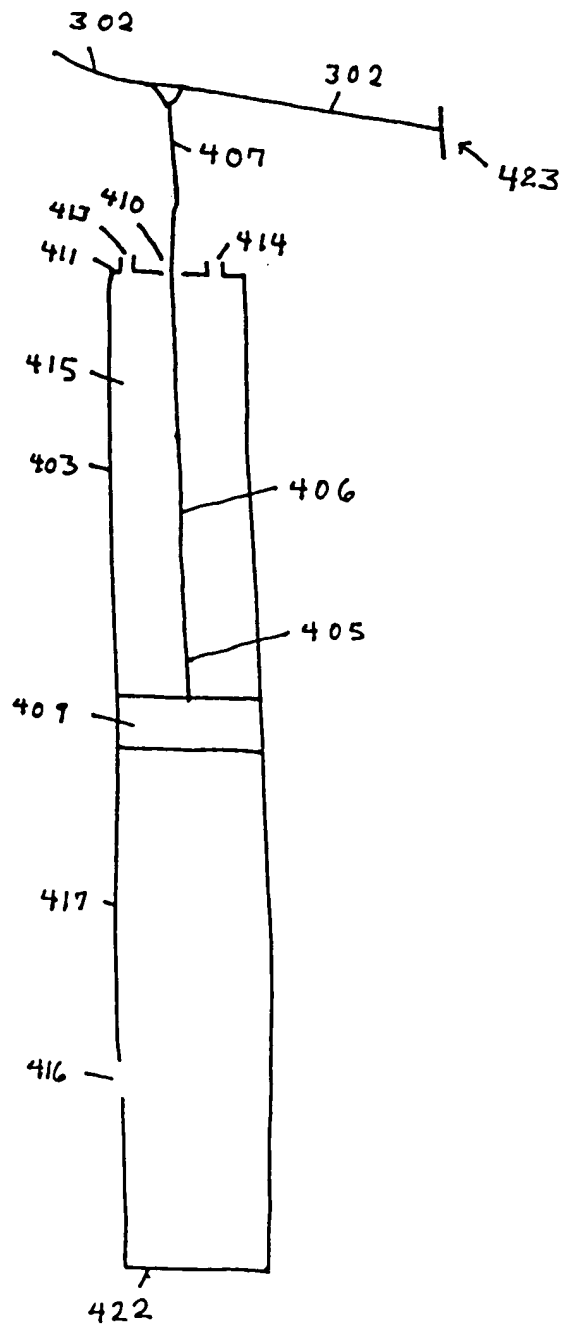


Figure 6

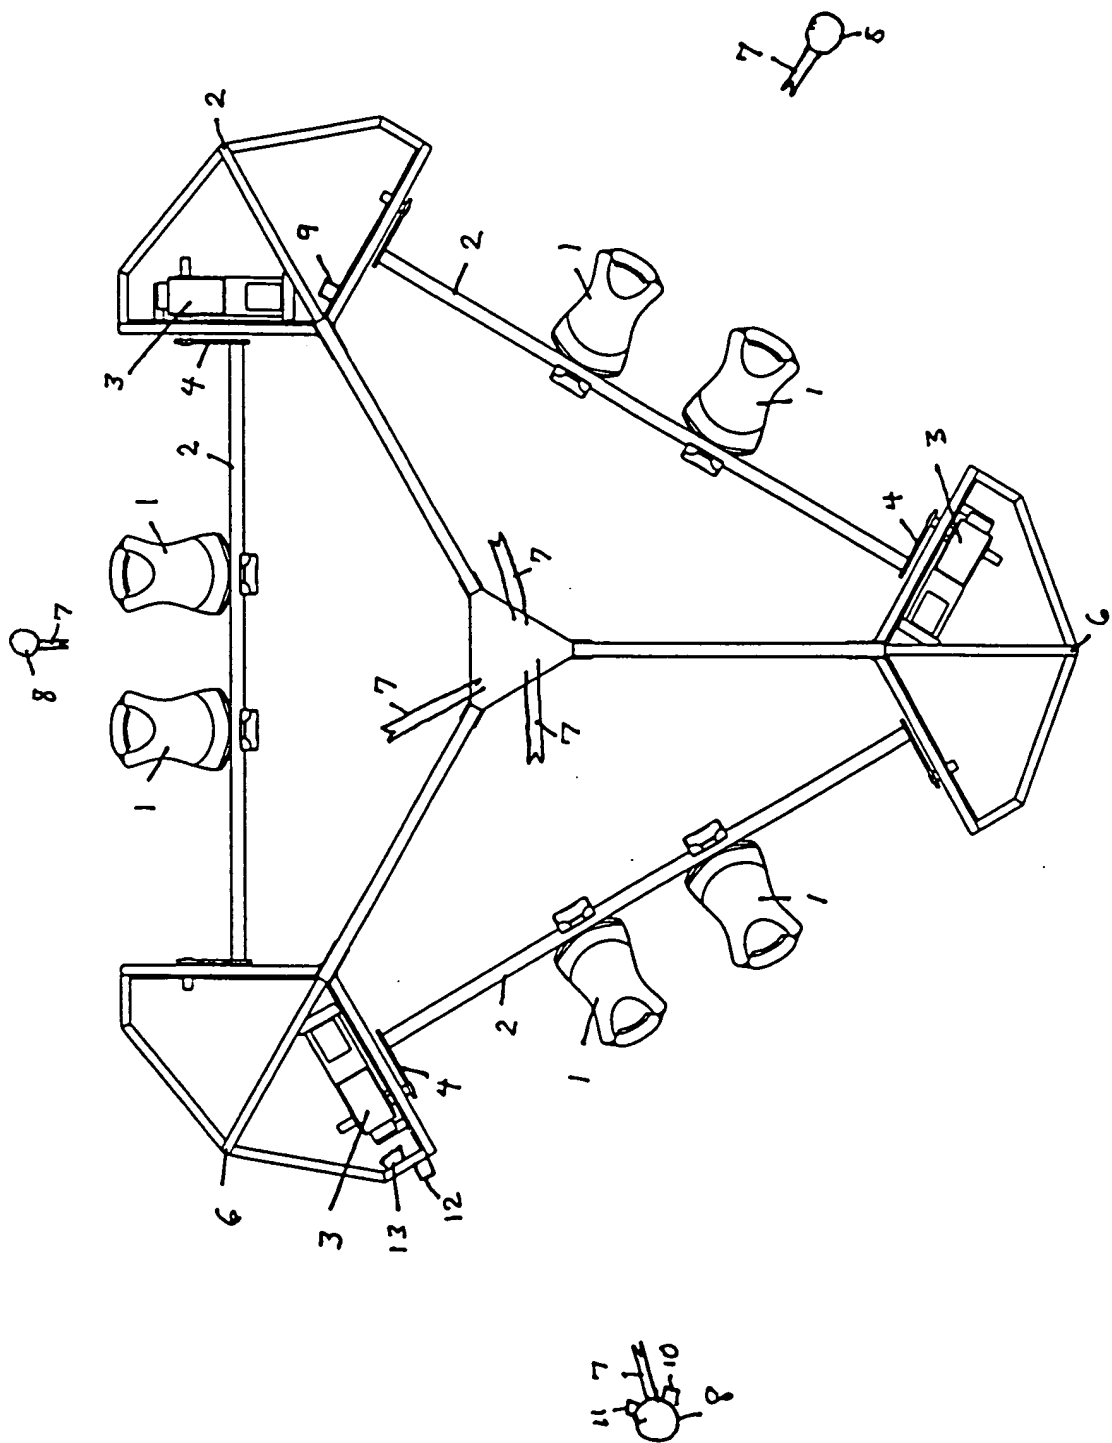


Figure 7





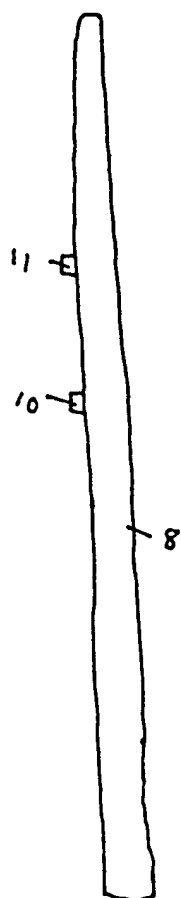


Figure 9

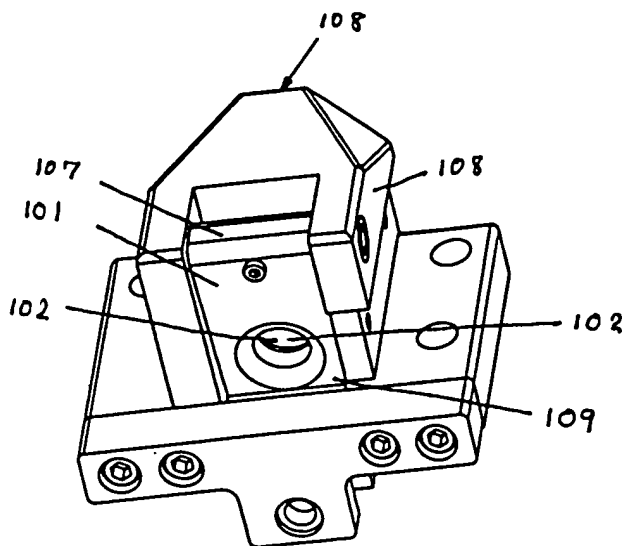


Figure 10





FIG. 13 is a perspective view of the device 100 in a retracted position.

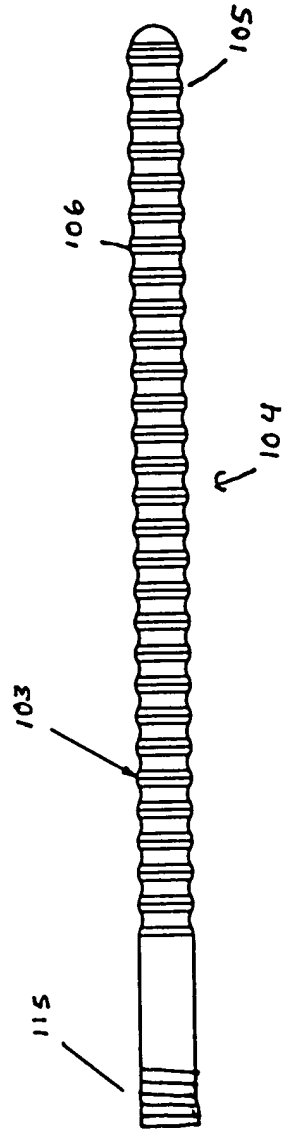



Figure 13



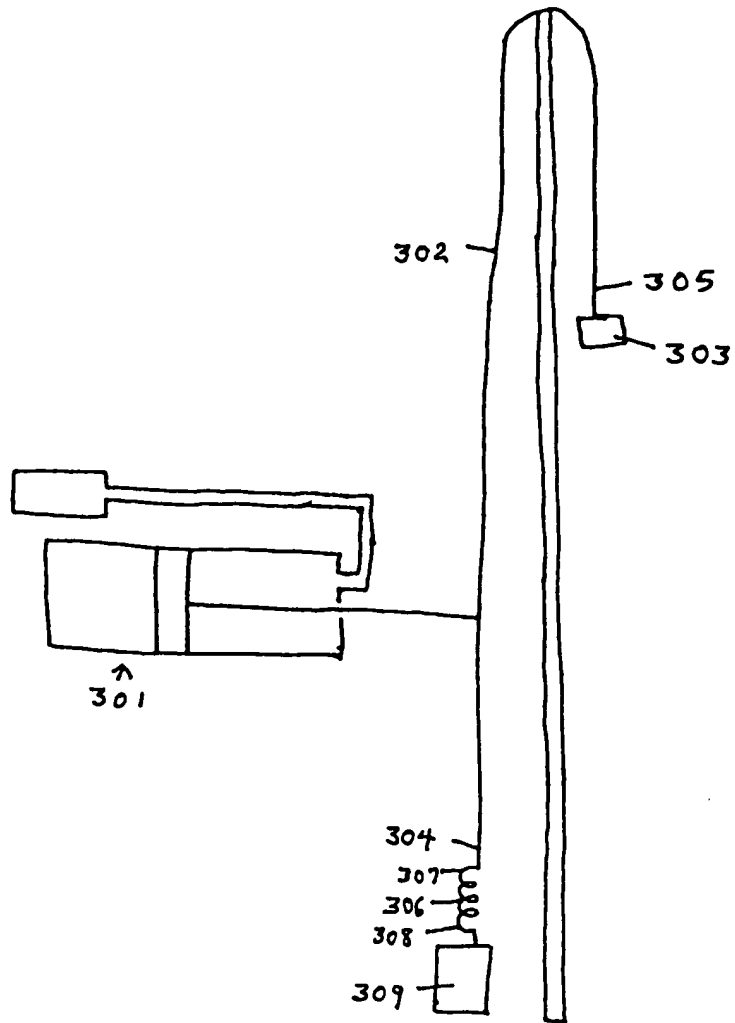


Figure 14

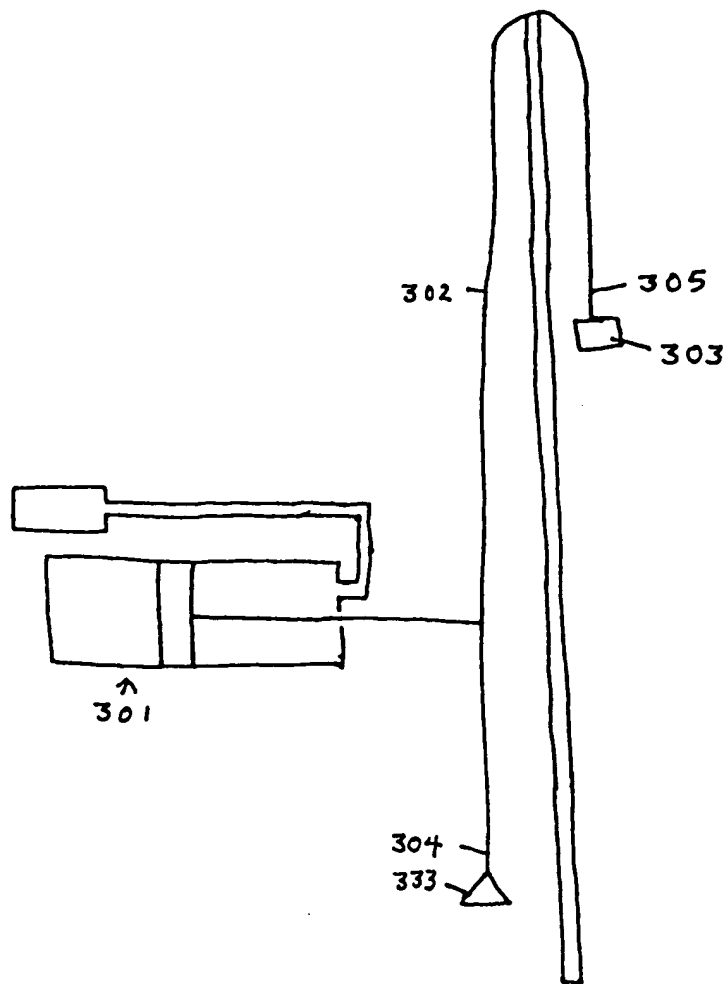


Figure 15

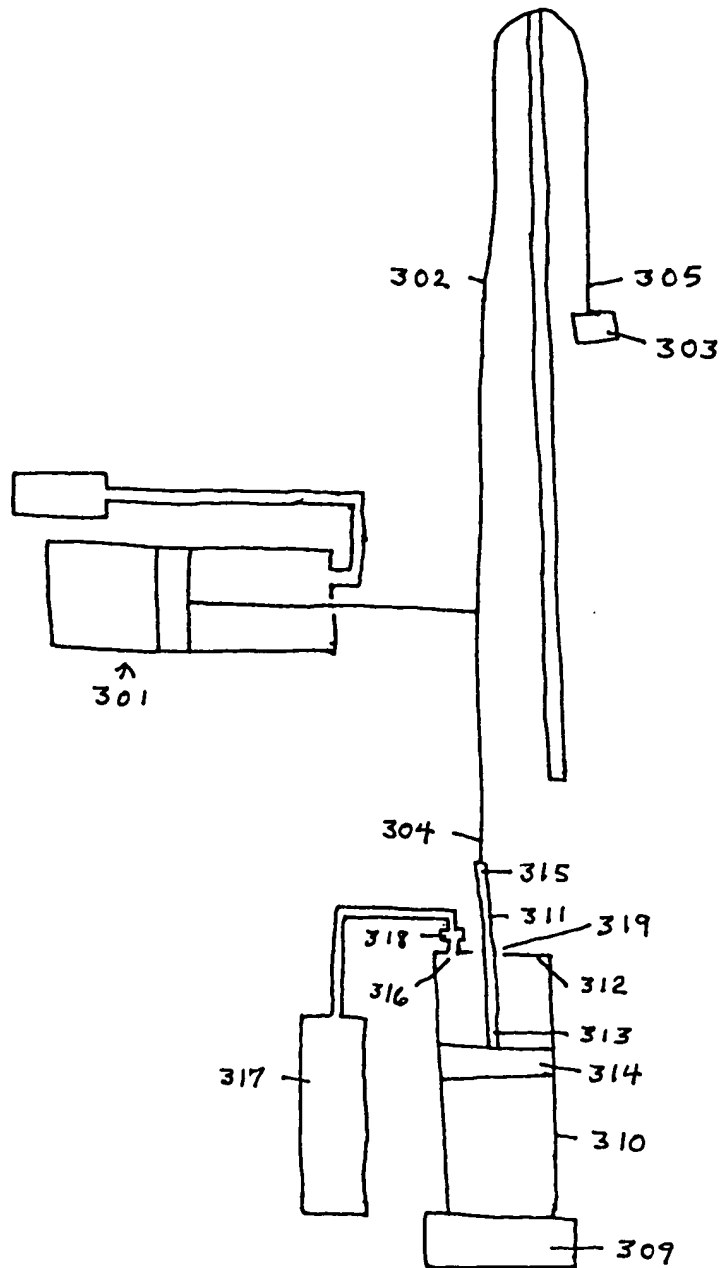


Figure 16



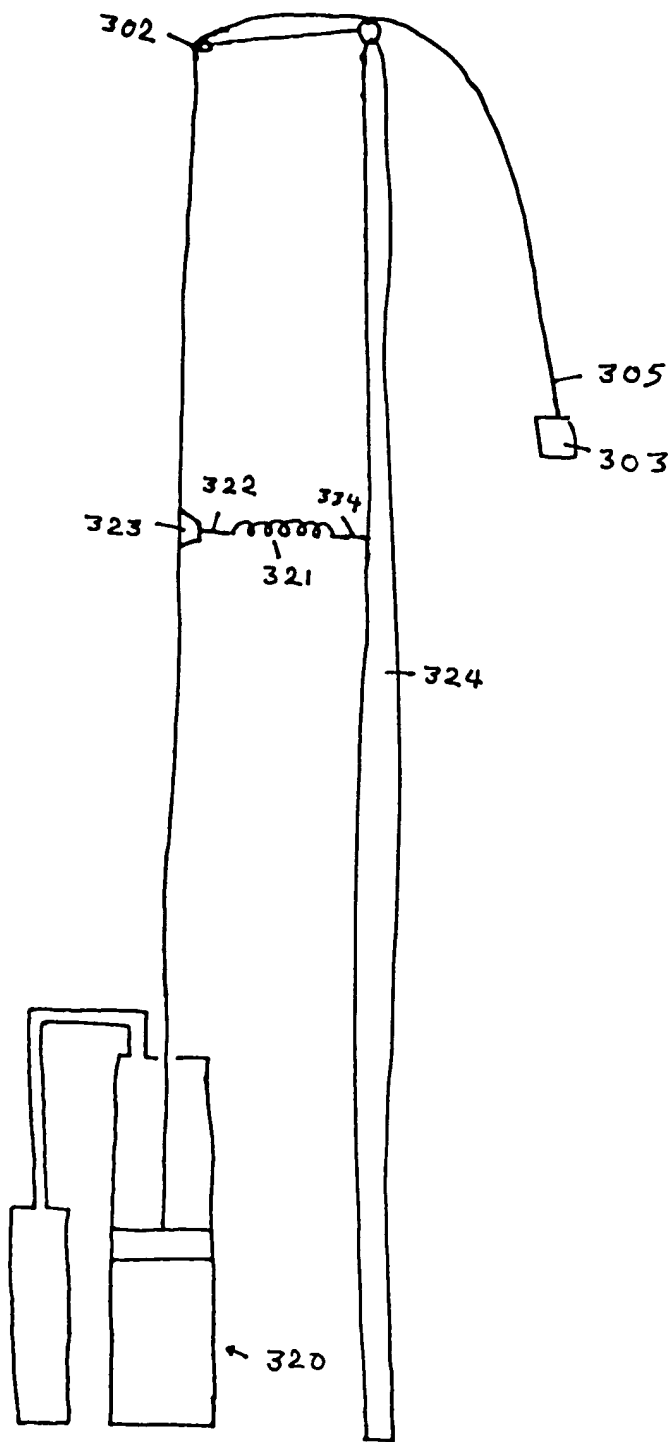



Figure 17

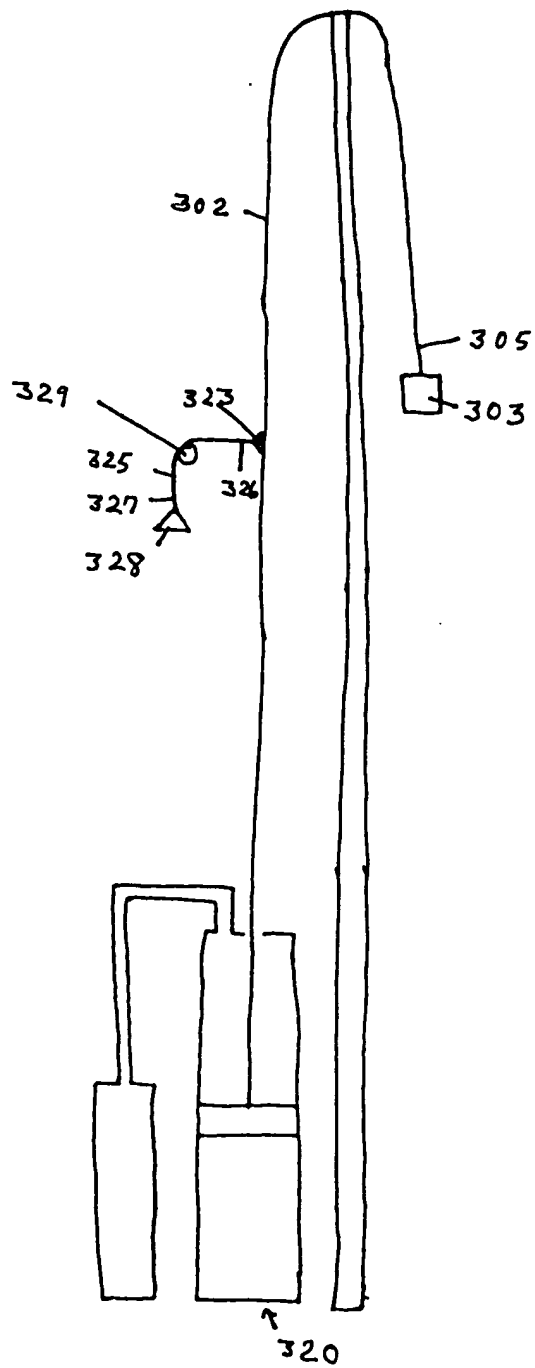


Figure 18

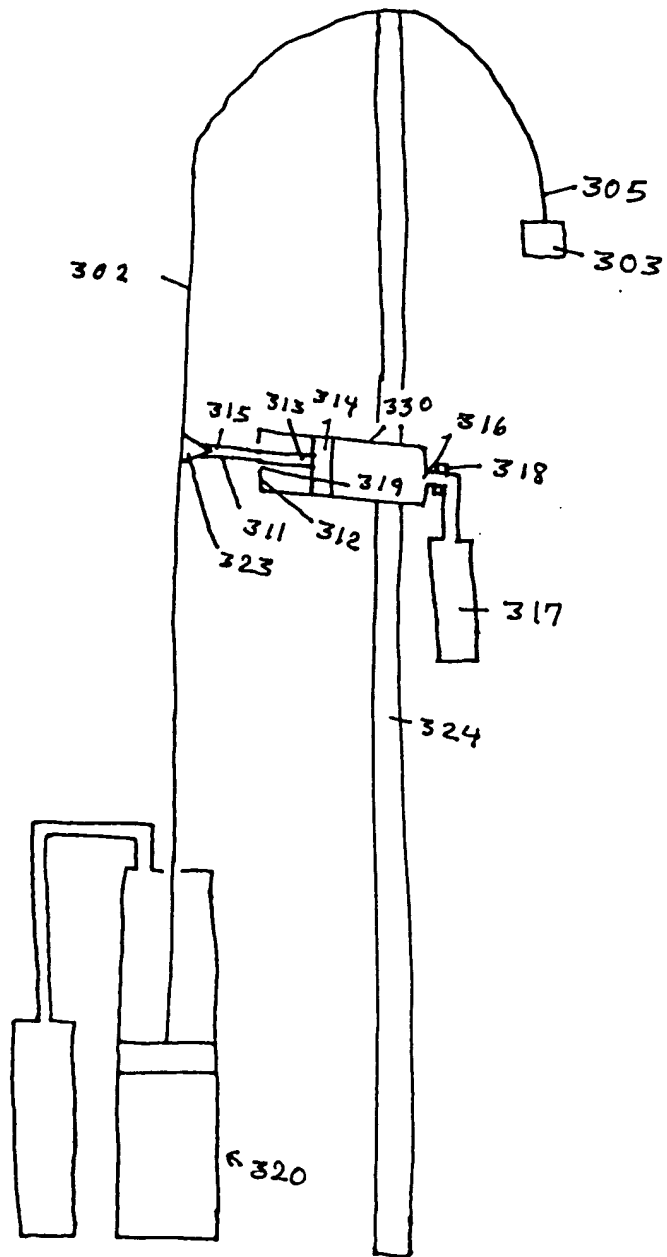


Figure 19

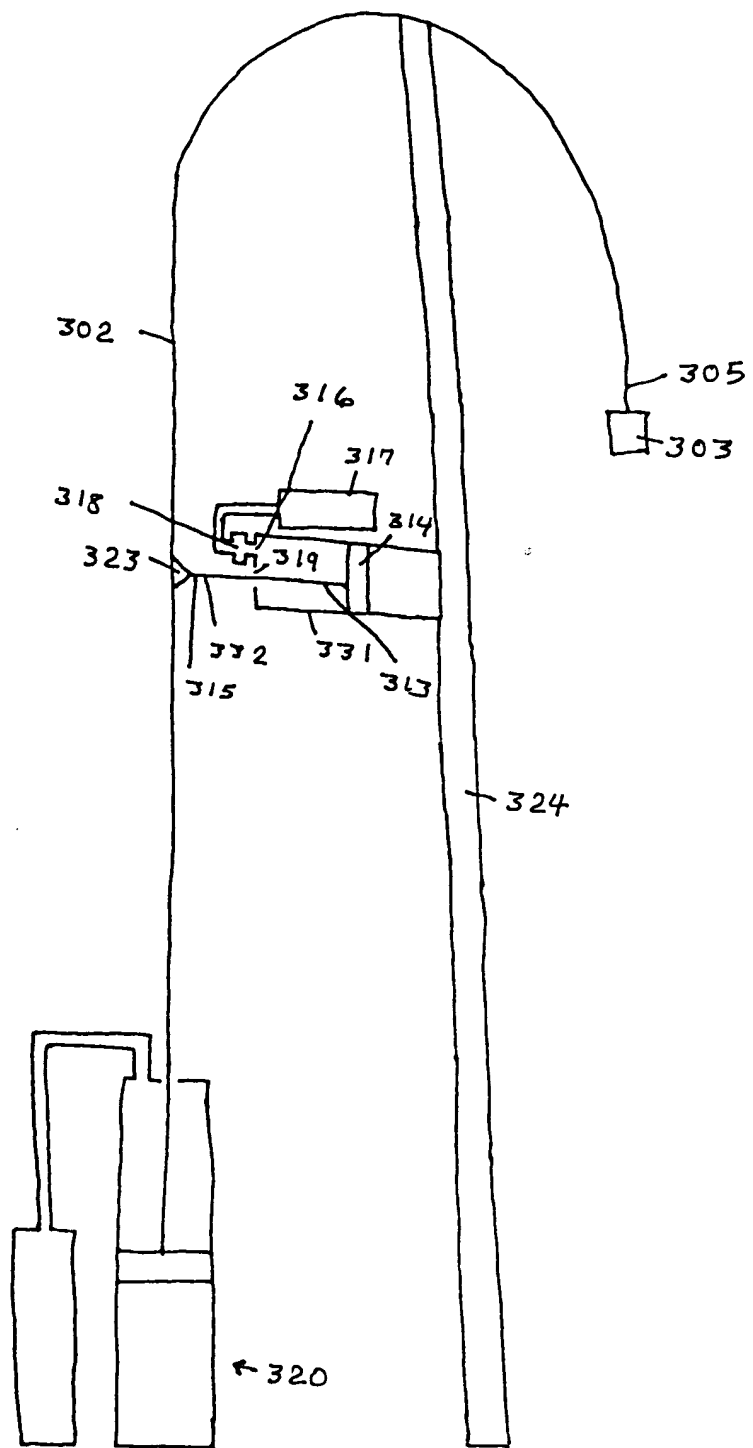


Figure 20

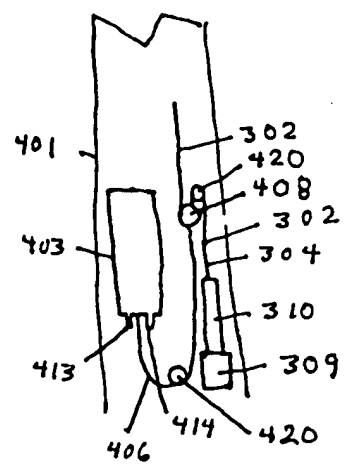
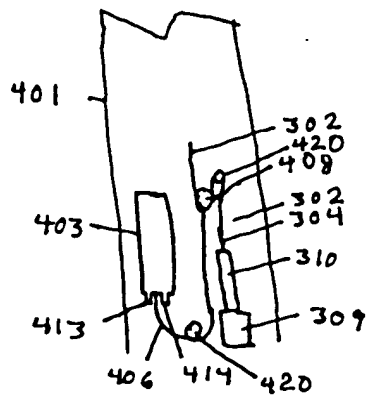
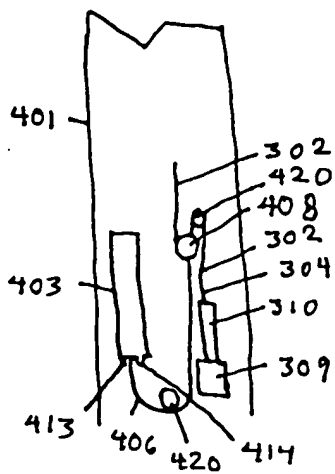
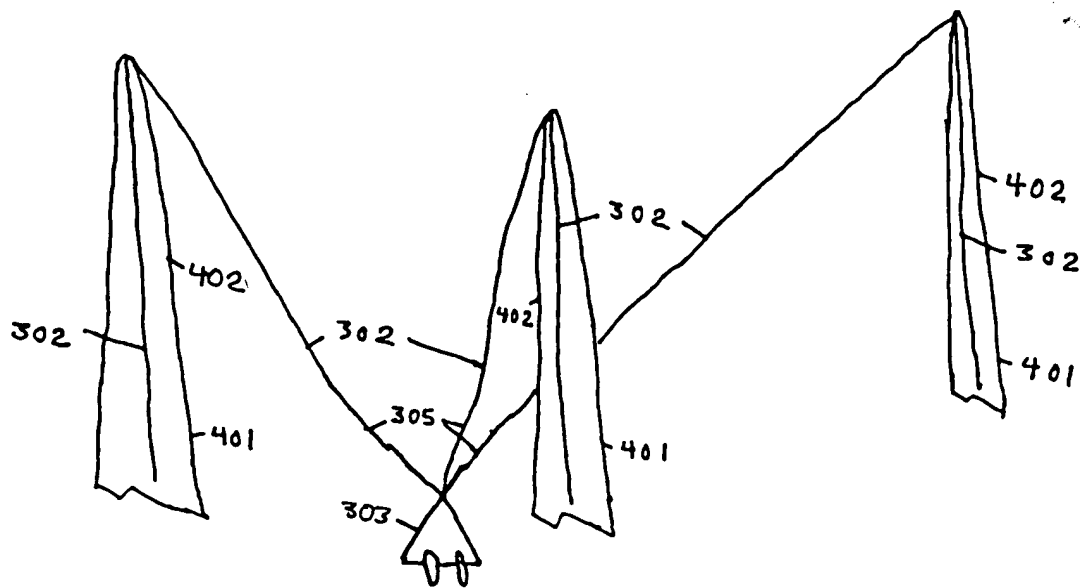


Figure 21